

Product:

Test Particles

BS-Partikel GmbH

Bahnstr. 10


D-65205 Wiesbaden

Phone: +49/611/7-888-999

Fax: +49/611/97-218-44

Email: support@BS-Partikel.de

URL: http://www.BS-Partikel.de



Catalog Number:

Te0700-25

Lot No.:

Te290.109

"Test Particles" are aqueous dispersions generally used to be applied for experiments, evaluations or simulations of specific particle situations (e.g. filter retention tests/-efficiency, studies of flow characteristics, etc.).

"Test Particles" are **not** designed for calibration of particle sizers. For this purpose we recommend our certified particle size standards.

Solid Contents:

5%

Particle Diameter (Mode):

$x_N = 6.5\mu\text{m} \pm 0.2\mu\text{m}$

$x_V = 6.5\mu\text{m} \pm 0.2\mu\text{m}$

Relat. Standard Deviation (C.V.): 4.9% rel. to x_N

Refractive Index: 1.59 (25°C, 589nm)

Polymer Density: 1.05 g/ml



Chemical Composition:

Poly(styrene-co-divinylbenzene)

water, surfactants (<0.1%), preservatives (<0.05%)

Particle Sizing System:

Single optical particle sizing system "Syringe", Markus Klotz GmbH, Bad Liebenzell - Germany

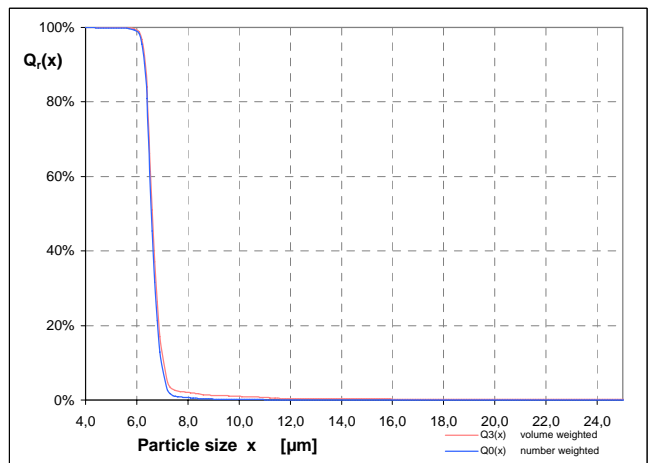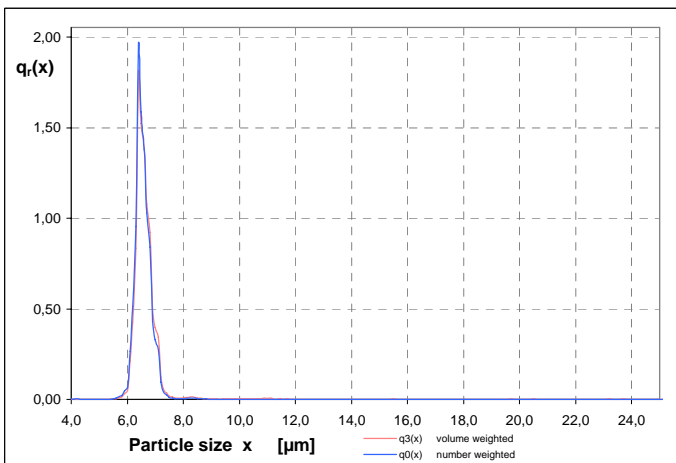

where is:

$$q_0 = (N_1 - N_2) / (N_{\text{all}} \cdot dx)$$

dx: channel width

$$q_3 = (V_1 - V_2) / (V_{\text{all}} \cdot dx)$$

$$Q_0 = 100 \cdot N_i / N_{\text{all}}$$

N_i and V_i : number and volume of all particles $\geq x_i$

$$Q_3 = 100 \cdot V_i / V_{\text{all}}$$